ANALIZA BIAŁEK

100014874

Laboratory of Analysis

Client: Forge Peptides
Order number: 100014874
Name: MIXING WATER
Number of samples: 1 vial

Batch number: ------
Recive date: 2026-05-25
Start date: 2026-05-26
End date: 2026-06-08

Sample identification


Tests	Method of taking a sample	Form
Benzyl Alcohol Microbiological	Sample provided by customer	Transparent liquid in a glass vial

Results

Substance	Sample name	Content	Purity
Benzyl Alcohol	MIXING WATER 10ML	0,95%	------

Test	Sample name	Result
TYMC	MIXING WATER 10ML	PASS
TAMC	MIXING WATER 10ML	PASS
Presence of presumptive Escherichia Coli	MIXING WATER 10ML	NOT DETECTED
Presence of Salmonella Spp.	MIXING WATER 10ML	NOT DETECTED

Photo of the test sample

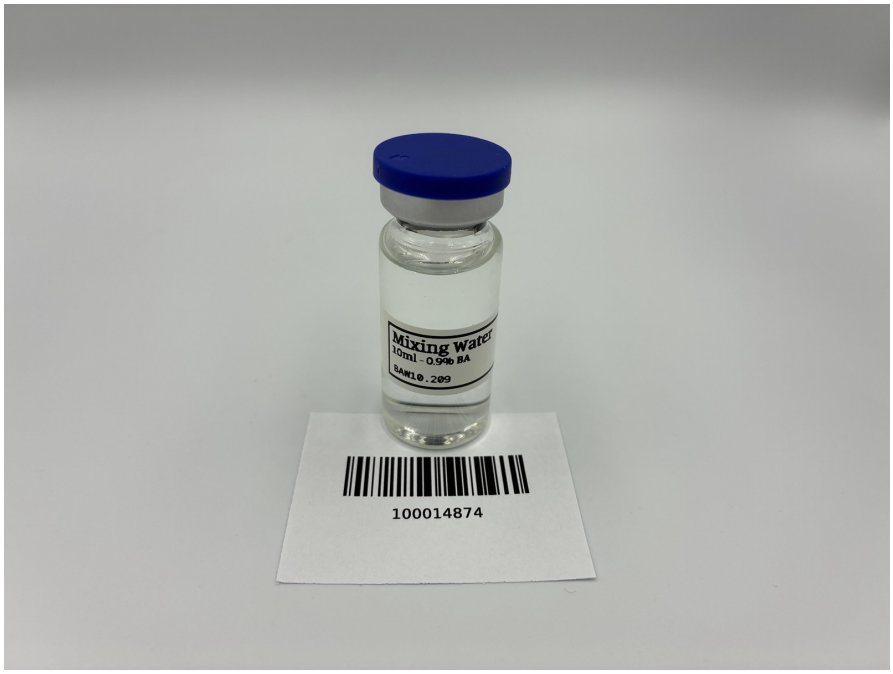

Password

F9L4P52A

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając