ANALIZA BIAŁEK

100014880

Laboratory of Analysis

Client: Forge Peptides
Order number: 100014880
Name: SEMAX/ SELANK
Number of samples: 1 vial

Batch number: ------
Receive date: 2026-05-25
Start date: 2026-06-05
Enda date: 2026-06-08

Sample identification

Substance	Method of taking a sample	Form
Semax, Selank	Sample provided by customer	White powder in glass vial


Results

Substance	Sample name	Content	Purity
Semax	SEMAX/ SELANK 20MG	9,94mg	99%
Selank	SEMAX/ SELANK 20MG	10,64mg	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H20 and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its concentration, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05 mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

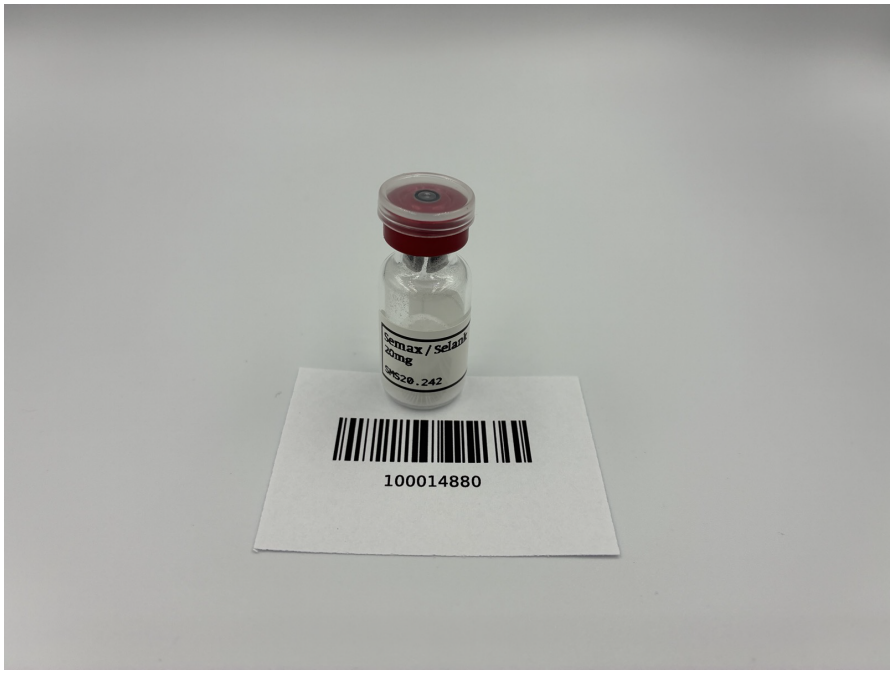

Password

7AK98E2A

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875


Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

100014880

Chromatogram

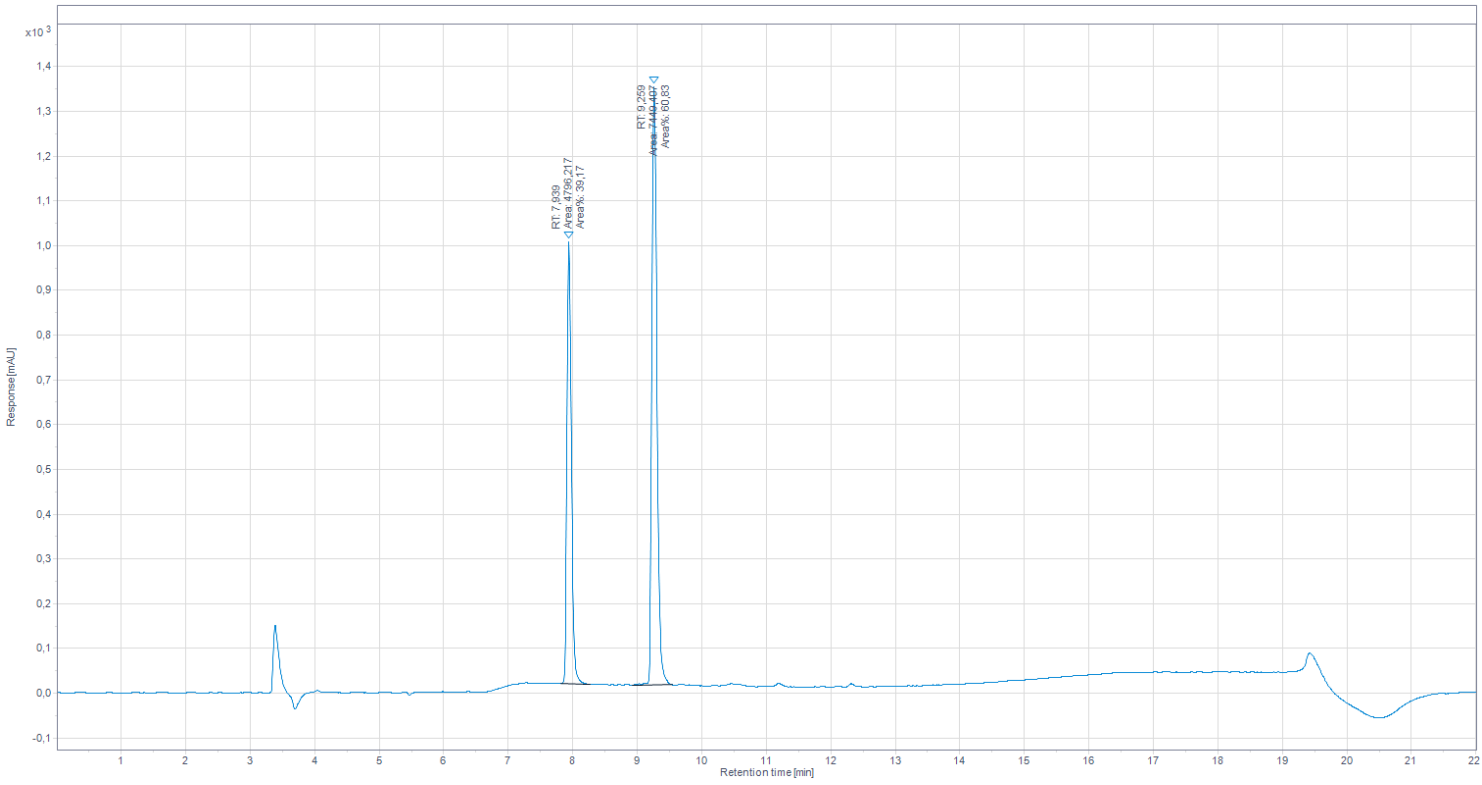

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

7AK98E2A

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając